



HOME NURSE CALL SYSTEM

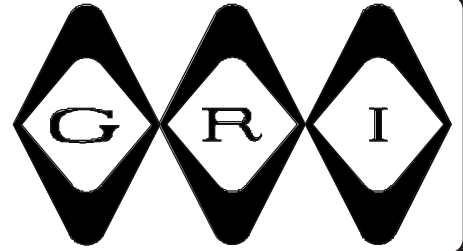

- ◆ Instant Alarm
- ◆ Signalling Device
- ◆ Self Contained
- ◆ Local Alarm and Flashing LED
- ◆ 2 Form C Relays
- ◆ Microprocessor Controlled
- ◆ Low Battery Indicator

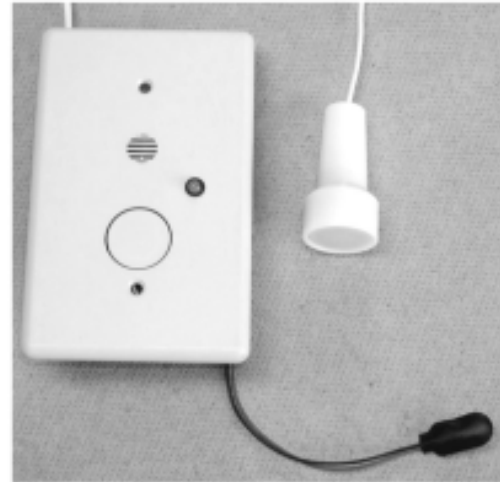

NC-20

APPLICATION:

The NC-20 is designed as a signaling device for use as a self contained Home Nurse Call System. The GRI Model NC-20 will sound a local alarm and flash an LED indicator, should anyone press the supplied (GRI CB-20) Call Button. The GRI NC-20 is also equipped with a form C relay output connections for use with external signaling devices.

DESCRIPTION:

The GRI Home Nurse Call System uses a microprocessor to monitor the open loop momentary push button (Call Button), the reset/cancel button, the supply voltage and provides control for sounder, LED and relay outputs. The Nurse Call System is set to alarm the instant the Call button is depressed. The sounder will continue to sound until the reset/cancel button is depressed. Other features for the NC-20 would include an adjustable sounder volume, power/alarm LED indicator, low battery indicator and (2 form C relay) contacts for control of external devices.

The C form relay contacts close 45 seconds after the alarm sounds. This allows for caregivers to respond and cancel before the external communication devices notify additional responders. (The external communication device is not supplied.)

GEORGE RISK INDUSTRIES, INC.
GRI PLAZA
KIMBALL, NE 69145



MADE IN U.S.A.

TOLL-FREE 1-800-445-5218
TOLL-FREE 1-800-523-1227
(308) 235-4645
FAX (308) 235-3561
E-MAIL: grisales@megavision.com
WEB SITE: www.grisk.com



HOME NURSE CALL SYSTEM

INSTALLATION WIRING DIAGRAM

For Multiple
Call Buttons

If more than one Call Button is used, the switches should be connected in parallel as in Figure 1.


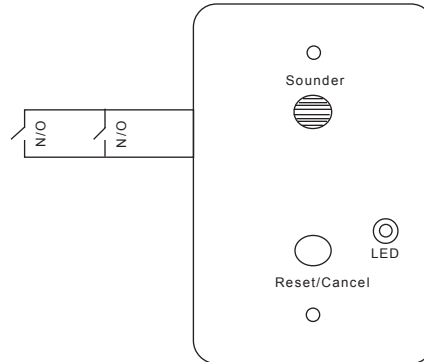


Figure 1. Wiring Diagram

Figure 2.
Terminal
Connections
& Jumpers

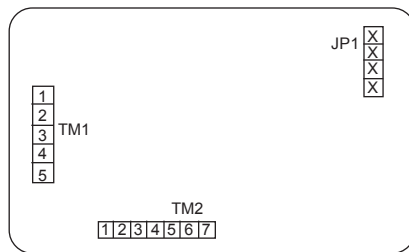

TERMINAL TM1

1. External Power (+)
2. Ground
3. Remote Reset/Delay Switch
4. Call Button -
5. Call Button +

TERMINAL TM2

1. Relay N/O
2. Relay Common
3. Relay N/C
4. Relay N/O
5. Relay Common
6. Relay N/C

Sounder Volume Control JP-1

<input checked="" type="checkbox"/>	Full Volume
<input type="checkbox"/>	
<input type="checkbox"/>	
<input type="checkbox"/>	
<input checked="" type="checkbox"/>	3/4 Volume
<input type="checkbox"/>	
<input type="checkbox"/>	
<input type="checkbox"/>	
<input checked="" type="checkbox"/>	1/2 Volume
<input type="checkbox"/>	

It is suggested applied voltage not exceed 15 VDC and surge protection, such as the GRI CS-1 Current Sensor, be used between the power supply and all GRI Low Voltage Alarms using external power.

NOTE: Unit will function at minimum 5VDC at a very limited sounder volume. This power level is considered total battery failure.

SPECIFICATIONS:

Battery Type	Standard 9 Volt
Battery Life	Approximately 3-6 months
External Power	9 to 12 VDC
Max. Input Power	40 mA
Recommended External Power Supply	12V DC 500 mA Regulated Output
Low Bat Mode	6.5V DC
Sounder Rated Switch	85 dB at 10 Ft. (3.5 M) Open Loop

Relay Contacts

Nominal Switching Capacity	2A 30 VDC
Max Switching Power	60 Watts
Max Switching Current	2 Amps

WARRANTY: One year against workmanship, material and factory defects.

CONTACT YOUR G.R.I. DISTRIBUTOR OR CALL:

GEORGE RISK INDUSTRIES, INC.
GRI PLAZA
KIMBALL, NE 69145



MADE IN U.S.A.

TOLL-FREE 1-800-445-5218
TOLL-FREE 1-800-523-1227
(308) 235-4645
FAX (308) 235-3561

E-MAIL: grisales@megavision.com
WEB SITE: www.grisk.com